

BATTERY REPLACEMENT

When the battery becomes weak the meter will display “-”. When the low battery indicator appears, the battery has only about 50 hours of working time left. A low battery will result in unreliable measurements. Prompt battery replacement is required.

Battery replacement must only take place in a non-hazardous area using an alkaline 9V battery.

Turn the meter off, slide the battery compartment cover located at the rear of the meter off and replace the 9V battery with a new one. Make sure the battery contacts are fully engaged in the connector, seat the battery in its compartment and replace the cover.

OPTIONAL ACCESSORIES

M10031B	1413 $\mu\text{S}/\text{cm}$ (1.41 mS/cm) calibration solution, 20 mL sachet (25 pcs)
M10032B	1382 mg/L solution, 20 ml sachet (25 pcs)
M10038B	6.44 g/L solution, 20 ml sachet (25 pcs)
M10039B	5000 $\mu\text{S}/\text{cm}$ (5.00 mS/cm) calibration solution, 20 mL sachet (25 pcs)
MA950	Portable meter wall mounting kit
SE-510	EC/TDS probe w/DIN connector and 1m cable
SE-520	EC/TDS probe w/DIN connector and 1m cable

CERTIFICATION

Milwaukee Instruments conform to the CE European Directives.

Disposal of Electrical & Electronic Equipment. Do not treat this product as household waste. Hand it over to the appropriate collection point for the recycling of electrical and electronic equipment.

Disposal of waste batteries. This product contains batteries. Do not dispose of them with other household waste. Hand them over to the appropriate collection point for recycling.

Please note: proper product and battery disposal prevents potential negative consequences for human health and the environment. For detailed information, contact your local household waste disposal service or go to www.milwaukeeinstruments.com (USA & CAN) or www.milwaukeeinst.com.



RoHS
COMPLIANT



RECOMMENDATION

Before using this product, make sure it is entirely suitable for your specific application and for the environment in which it is used. Any modification introduced by the user to the supplied equipment may compromise the meter's performance. For your and the meter's safety do not use or store the meter in hazardous environment. To avoid damage or burn, do not perform any measurement in microwave ovens.

WARRANTY

These instruments are warranted against defects in materials and manufacturing for a period of 2 years from the date of purchase. Probe is warranted for 6 months. This warranty is limited to repair or free of charge replacement if the instrument cannot be repaired. Damage due to accidents, misuse, tampering or lack of prescribed maintenance is not covered by warranty. If service is required, contact your local Milwaukee Instruments Technical Service. If the repair is not covered by the warranty, you will be notified of the charges incurred. When shipping any meter, make sure it is properly packaged for complete protection.


ISTMW402_07_20



USER MANUAL

MW301, MW302, MW401, MW402

PRO EC/TDS Portable Meter

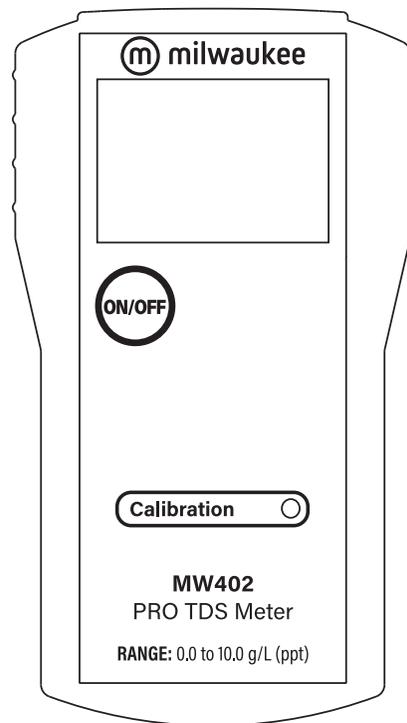


milwaukeeinstruments.com (USA & CAN)
milwaukeeinst.com

milwaukee


OPERATION

- The meter is supplied complete with a 9V battery.
- Slide off the battery compartment cover on the back of the meter. Install the battery into the battery clip connector while observing polarity.
- Connect the probe to the meter securely by aligning the pins with the plug in.
- Make sure that the meter has been calibrated before taking any measurements (see Calibration Procedure).
- Immerse the tip (4 cm) of the EC/TDS probe into the sample. If possible use plastic beakers or containers to minimize any EMC interference.
- Turn the instrument on by pressing the ON/OFF key.
- Wait for the temperature sensor to reach the thermal equilibrium before taking any measurements.
- After use, the instrument should be switched off and the probe should be cleaned and dried. Whenever needed, use alcohol for better cleaning.

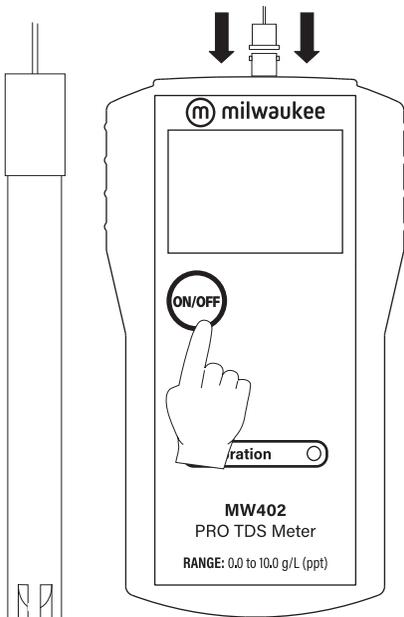

CALIBRATION PROCEDURE

- Clean the probe with alcohol and let it dry.
- Open a sachet of conductivity calibration solution (see Specifications) and immerse the probe making sure that the metal pins are completely submerged.
- Wait until the thermal equilibrium is reached and the reading is stable.



- Adjust the calibration trimmer on the front panel of the instrument with the supplied screwdriver until the display shows:
 - “1410 μ S” for **MW301**
 - “1410 μ S” for **MW302**
 - “1380 mg/L” (ppm) for **MW401**
 - “6.4 g/L” (ppt) for **MW402**



- The calibration is now complete and the meter is ready for use.
- The instrument should be re-calibrated at least once a month, or whenever the probe or battery is changed

SPECIFICATIONS

RANGE/RESOLUTION	
MW301	0 to 1990 μ S/cm / 1 μ S/cm
MW302	0.0 to 10.0 mS/cm / 0.1 mS/cm
MW401	0 to 1990 mg/L (ppm) / 1 mg/L
MW402	0.0 to 10.0 g/L (ppt) / 0.1 g/L
ACCURACY	
	\pm 2% Full Scale
CONVERSION FACTOR	
MW401	0.5
MW402	0.5
CALIBRATION SOLUTIONS	
MW301	1413 μ S/cm = 1.41 mS/cm (M10031B)
MW302	1413 μ S/cm = 1.41 mS/cm (M10031B)
MW401	1382 mg/L (M10032B)
MW402	6.44 g/L (M10038B)
CONDUCTIVITY PROBE	
MW301 & MW401	SE-510 (included)
MW302 & MW402	SE-520 (included)
TEMP. COMPENSATION	
	Automatic, from 5 to 50°C
ENVIRONMENT	
	0 to 50°C, 95% RH max.
BATTERY TYPE	
	1 x 9V alkaline (included)
BATTERY LIFE	
	approximately 300 hours of use
DIMENSIONS	
	143 x 80 x 32 mm
WEIGHT	
	220 g (with battery) meter only